

Stratus Turn™



User Manual

Doc. #: _____ Rev. Date: _____ Rev.: _____

Sizewise®
Designed to heal

Table of Contents

Definition of Symbols	4
Manual Definitions.....	4
Warnings and Cautions	5
Device Information.....	6
Description of the Device.....	6
Purpose of the Device.....	6
Indications for Use	6
Specifications	7
Unpacking and Set-Up Instructions	8
Unpacking / Parts Breakdown	8
Operating Instructions	10
Modes of Operation	11
Patient Care Functions.....	12
Placing the Patient on the Mattress Surface	12
Positioning the Patient.....	12
Backrest Up or Fowler Position	12
Prone Position.....	13
Bedpan Placement & Removal.....	13
Removing the Patient from the Mattress Surface.....	13
Keypad Quick Reference.....	14
Maintenance	15
Air Filter/HEPA Filter.....	16
Mattress Cleaning Instructions.....	18
Mattress Top Cover:.....	19
Laundry Instructions:	19
Mattress Base:	20
Air Therapy Internal Mattress Components:.....	20
Cleaning Blood and Other Excretions:.....	20
Control Unit/Blower Cleaning Instructions:	21
Safety Tips.....	22
Seven Zones of Bed Rail Entrapment	22
Storage and Disposal	23
Important Safety Instructions	24

Electromagnetic Compatibility (EMC) 25
Troubleshooting..... 30
Frequently Ordered Parts..... 31
Warranty Information..... 32

Definitions and Symbols

Definitions

Throughout this manual different type fonts and symbols are used to aid user readability and understanding of the content. Below are some examples.

Standard Text: Used for regular Information.

Bold Face Text: Emphasizes a word or phrase.

NOTE: Sets apart special information or important instruction clarification.

Symbols



Electrical Shock Hazard Warning: This symbol is intended to alert the user to the presence of electrical shock hazards. It's important to follow all instructions and special procedures to avoid electrical shock to the operator, care provider and/or patient.






Warnings/Cautions: This symbol is intended to alert the user to the presence of important operating, maintenance or servicing instructions. Disregarding a warning could result in patient and/or user injury as well as damage to equipment.

 Warning/Attention		
Read and fully understand manual before operating. Failure to follow operating instructions could result in death or serious injury.		Lisez et comprenez entièrement le manuel avant utilisation. Le non-respect des instructions d'utilisation peut entraîner la mort ou des blessures graves.
27008710, Rev. 1.0		

Manufacturer's Label

UDI Information on separate label located on product near this label.

Sizewise Manufacturing	ETL CLASSIFIED  US Intertek 3101425		Class I Electrical Equipment	 Type B	Indoor Use Only MADE IN USA
Legal Manufacturer: Raye's, Inc. d/b/a Sizewise Manufacturing 206 Jefferson Street Ellis, KS 67637			Medical Electrical Equipment Conforms to: AAMI Std. ES60601-1, IEC Std. 60601-1-6 Certified to: CSA std. C22.2 No. 60601-1		
Model: Serial #: Manufacture Date: Duty Cycle: Electrical Rating:					
27510711 Rev. 5.0					

Power Cord Label



This symbol signifies that the device is properly protected from electrical shock.




This symbol marks the location of the leakage test point screw.




Replace fuse as marked

This symbol marks the location and specification of the fuse.

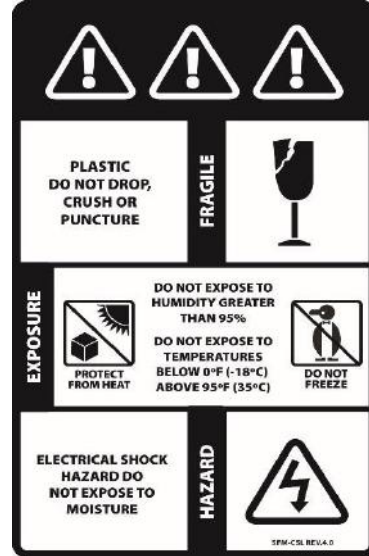

The hazards and warnings are indicated on the shipping container by this label.

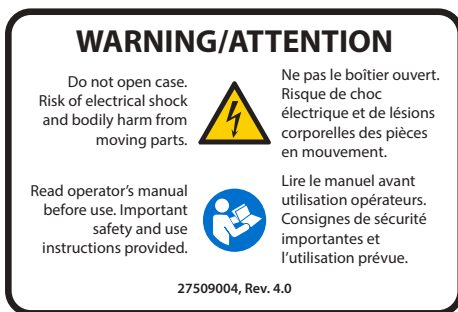

ELECTRICAL SHOCK HAZARD WARNING:
Do not open case for risk of electrical shock.

Device Information

Description of the Device

The SIZEWISE STRATUS TURN® Clinically Effective Low Air Loss Mattress System is comprised of a specialized inflatable air bladder (air mattress) and an electrically powered Control/Blower Unit.

Purpose of the Device

The purpose of the SIZEWISE STRATUS TURN® is to provide therapeutic benefit to patients at risk, or suffering from pressure ulcers.

The SIZEWISE STRATUS TURN® also has operator controls that allow the operator or caregiver to adjust the patient's body weight pressure distribution by increasing and decreasing of pressure in defined areas of the mattress on a timed basis. This results in an angular change of the patient's body such as the left shoulder and hip being lowered below that of the right shoulder and hip, resulting in a turn.

The active component that has contact with the patient is a specialized, multi-cell air mattress sized to fit a standard medical bed frame. The air mattress serves as a replacement mattress and is equipped with 4 air hoses with connectors that mate with the Blower / Control Unit. The Control Unit is a self-contained, totally enclosed module that hangs by hinged hooks on the bed frame. **NOTE: Do not place control unit under bed.**

The SIZEWISE STRATUS TURN® Mattress System has a detachable hospital-grade electrical cord and a control panel with selector switches and indicator lights. The switches and indicators are protected under a flexible membrane to keep out liquid spills and enhance clean-up and sanitation. Inside the Control/Blower Unit is a variable output blower, a valve motor and air valves that allow the air mattress to operate in static mode or provide cyclic pressure variations within the mattress. There is also a printed circuit board, which provides the electrical controls.

Indications for Use

The SIZEWISE STRATUS TURN® is a therapeutic mattress that provides both active or reactive pressure redistribution and clinically effective low air loss therapy. When mobility, moisture and/or inactivity are healthcare concerns, it is indicated for the prevention and treatment of pressure ulcers and other skin related injuries.

Specifications

SIZEWISE STRATUS TURN®

Control Unit/Blower

- **Mode of Use**For Indoor Use Only
- **Duty Cycle**.....Continuous
- **Controller Dimensions**..... (LxWxH) 6”(15 cm) x 16”(41 cm) x 10.5”(27cm)
- **Controller Weight**..... 11 lb. (4.98 kg)
- **Operating Temperature**..... -18°C to 35°C (0°F to 95°F)
- **Alternating Low Air Loss** 3 minutes-90 minutes
- **Alarms** Power Failure and Low Pressure

Electrical

- **Rated Voltage/s** 110 Volts and 220 Volts
- **Rated Frequency 110 Volts/Input Power** 60Hz/120 Volts
- **Rated Frequency 220 Volts/Input Power** 50Hz/230 Volts
- **Degree of Shock Protection**.....Type B
- **Maximum Relative Humidity**95%
- **Storage Temperature**-18°C to 35°C (0°F to 95°F)
- **Environmental Conditions** Product must be stored and transported in packaging free of moisture and dust
- **Power Cord**16’ (5 meters) detachable with hospital-grade plug
- **Fuses 110 Volt**T300mA 250V...T5A 250V
- **Fuses 220 Volt**T2.5A 250V
- **Power Failure Alarm** YES

Mattresses

- **Inflated Dimensions 35”**(LxWxH) 80”(203.2cm) x 35”(88.9cm) x 8”(20.3cm)
- **Weight Capacity 35”in therapy**..... up to 350 lb. (158.76 kg)
- **Weight Capacity 35”in static/pulse therapy**up to 600 lb. (272.15 kg)
- **Weight Capacity 39”/42”in therapy** up to 450 lb. (204.11 kg)
- **Weight Capacity 39”/42”in static/pulse therapy** up to 1000 lb. (453.59 kg)
- **Top Cover Material** 70 Denier Polyurethane Coated Nylon Taffeta

Unpacking and Set-Up Instructions

The two main components of the SIZEWISE STRATUS TURN® Mattress Replacement System are a specialized air inflatable bladder (Air Mattress) and an electrically powered Control/Blower Unit.

Unpacking / Parts Breakdown:

Parts:

- Control Unit/Blower
- Detachable Power Cord (Hospital Grade)
- Clinically Effective Low Air Loss Mattress Replacement
- Mattress Cover



Control Unit/Blower



Detachable 16'
Hospital Grade
Power Cord



Clinically Effective
Low Air Loss
Mattress with
Cover

Unpacking Instructions: Remove the products from the packing material and examine for shipping damage. If damage is detected in shipping, contact the freight company and file a damage complaint immediately.

Environmental Conditions:



CAUTION: Keep out of direct sunlight.

DO NOT expose to temperatures below 0°F (-18°C) or above 95°F (35°C).

DO NOT expose to moisture or areas of humidity greater than 95%.

Beware of Electromagnetic Interference from Radio Wave Sources such as: Hand-held portable transceivers with the antenna mounted directly to the transmitting unit including citizen band (CB) radios, “walkie-talkies, security, fire and police transceivers, cellular telephones and other personal communication devices.

NOTE: Some cellular telephones and similar devices transmit signals while they are ON, even when not being used.

Directions for Mattress Placement: Replace the existing bed mattress with Clinically Effective Low Air Loss Mattress. Secure Air Mattress to the bed frame with straps provided.



Warning or Safety Instructions relating to setup: WARNING: (120V unit ONLY)
Make sure the power cord is plugged into a properly grounded hospital grade 120V A/C outlet.



Warning or Safety Instructions relating to setup: WARNING: (220V unit ONLY)
Make sure the power cord is plugged into a properly grounded hospital grade 220V A/C outlet.

Operating Instructions

The SIZEWISE STRATUS TURN® can be placed on any conventional bed used in hospitals, nursing homes or a home medical bed. The original bed mattress should be removed and stored in an appropriate place. The following steps should be completed in installing the system:

1. Remove standard mattress from the bed.
2. Replace standard mattress with the SIZEWISE STRATUS TURN®. (Be sure air tubing is at the foot end of the bed).
3. Strap air support mattress to bed frame on all four sides with straps provided.
4. Place the Control Unit/Blower on the footboard of the frame using the two hinged hooks located on the back of the unit.
5. Attach the air tubing to the Control Unit/Blower, being sure it snaps in tight. (Be sure air tubing is not kinked and is unobstructed).
6. Plug the Control Unit/Blower into a grounded hospital grade A/C outlet.
7. Turn the master power switch ON.
8. Press the AUTOFIRM button for quick inflation. (see keypad quick reference section)
9. Place the patient on the bed AFTER inflation to ensure the air cells do not become twisted or kinked.
10. After inflation, press the AUTOFIRM button again to exit Auto Firm mode. (If the Control Unit/Blower is left in Auto Firm mode for 10 minutes then it will automatically return to the previous mode of operation).

NOTE: See Keypad Quick Reference (table of contents) for further illustration.

Modes of Operation

1. Static Mode



- a. Press the Mode button until the Static option light comes on
- b. Set the desired comfort level with the Soft/Firm arrow buttons.

2. Fowler Mode




- a. When elevating the head section of the mattress, press the Fowler button to increase airflow for seat inflation.

3. Auto Fowler Attachment (optional)

- a. When elevating the head section of the mattress, Fowler mode will automatically turn on.



Auto Fowler attachment



This is where the Auto Fowler attachment connects to the control unit.

4. Pulsate Mode

- a. Press the Mode button until the Pulsate option light comes on.
- b. Set the desired cycle time with Cycle Time buttons (3-20 minutes).
- c. Set the desired comfort level with the Soft/Firm buttons.

5. Turning Mode

- a. Press the Mode button until Right Turn, Left Turn or Full Turn is illuminated, which ever mode you desire. At this setting the degree of rotation will be approximately 40 degrees.
- b. In Full Turn mode the control unit has a preset of 3-minute intervals. The intervals may be adjusted by depressing the cycle time button to desired time (3 to 20 minutes. 30, 45, 60, 75 or 90 minutes also.)
- c. To set comfort level press corresponding firm or soft button. There are 10 levels of firmness indicated by lighted bars located on the control panel.

NOTE: When the cycle time is showing “Hd” the control unit will hold the patient in the turn position until a caregiver physically changes the cycle time.



CAUTION: When the patient is placed in Turning Mode, pay close attention to IV lines and tubing to ensure there is enough length to accommodate a full rotation. IT is advised to monitor the patient for two to three complete rotations.

6. Lockout Feature

- a. After 3 minutes, if there are no changes to the Control Unit/Blower settings, the lockout feature will activate.
- b. Press and hold the Lockout button for 3 seconds to disengage the Lockout feature.

7. Quick Deflation or CPR Use

- a. Turn power OFF.
- b. Twist CPR plug on mattress to open.
- c. Remove the hoses from the Control Unit/Blower.

For Inquiries Call 1-800-814-9389

Patient Care Functions

Placing the Patient on the Mattress Surface

Place the patient on the mattress surface from a bed or stretcher with a transfer device. The mattress should be set in the Auto Firm mode. In order to ensure proper immersion and envelopment of the patient, the user should:

1. Position patient on surface in center of bed.
2. Initialize soft/firm settings on the Control Unit/Blower.
3. Wait a moment to allow internal sensors to activate pressure redistribution. Generally, depending on patient body makeup, initial pressure redistribution is complete in approximately 2-3 minutes.
4. Elevate the head of the bed to at least 30 degrees.
5. Unzip the mattress and visually inspect the height of the cells for sufficient inflation. There should be several inches between the patient and the frame of the bed. Adjust the air flow accordingly. Ask the patient if they can feel the bed frame beneath them. If yes, add air incrementally. Repeat until patient no longer feels the frame beneath them.
6. If the patient cannot reply verbally, unzip the mattress and visually inspect the height of the cells for sufficient air inflation. There should be several inches between the patient and the frame of the bed. Adjust the air flow accordingly.
7. CPR: The standards for life support recommended by the American Heart Association for performing CardioPulmonary Resuscitation (CPR) recommend a hard level surface for performing CPR, moving the person to the floor if possible. For performing CPR, place the CPR board, lower the head of the bed, position the patient on their back and follow standard CPR procedures of the facility.

In some cases, the mattress may include an auto-fowler feature. This means that when the head of the bed is greater than 30 degrees, the mattress will automatically increase the amount of air to the sacral area.

Positioning the Patient

When moving a patient the Control Unit/Blower should be in the Auto Firm Mode.

To reposition the patient, change the Control Unit/Blower to Auto Firm Mode. This makes the mattress surface firm and facilitates the repositioning of the patient with less strain on the care provider. When the patient has been repositioned, press auto firm to return to the previous setting.

NOTE: DO NOT leave a patient unattended on the mattress surface with the safety side rails in the down position. When leaving a patient, secure the safety side rails in the up position. Make sure the safety side rails are high enough to properly protect the patient when the mattress is fully inflated, while continuing to be mindful of the FDA guidelines on bed rail entrapment.

Backrest Up or Fowler Position

When the patient's backrest is elevated, it may be necessary to manually increase the mattress firmness to compensate for the additional weight placed in the center portion of the mattress.

Observe the patient for a short time after raising the backrest to make sure the buttocks and thigh areas are not “bottomed-out”.

Prone Position

DO NOT leave a prone patient on the mattress surface. If the patient is unable to move without help, the patient’s airway may be compromised. If the patient is to be kept prone for an extended period of time, consult a Sizewise representative for assistance.

Bedpan Placement & Removal

Position the patient’s hips over the center of the mattress. Using Static Mode, lower the pressure setting with the Firm/Soft button. Turn the patient into the side-lying position and place the bedpan.

The pressure in the center section of the mattress will lower to make inserting the bedpan easier. The firmness setting may be adjusted to increase the firmness of the center section after the pan is placed in position.

When the bedpan is to be removed, logroll the patient off the bedpan and remove it. Readjust the firmness level to the appropriate setting. Select Static mode and wait for the mattress to completely re-inflate before activating Alternate Pressure mode again.

NOTE: Always remove the bedpan before entering the Alternate mode.

Removing the Patient from the Mattress Surface

If the patient is to be removed with a transfer lift, set the Control Unit/Blower into Auto Firm mode. Allow the mattress to firm and position the patient into the lift. When the patient has exited the bed, the controller can be turned off.

If the patient can sit up and is mobile, lower the firmness level to the lowest setting and wait for the mattress to soften in the middle. The patient can sit up and the mattress will conform to the body making a more stable platform for patient egress. When the patient has exited the bed, the controller can be turned off.

Keypad Quick Reference



Lockout
Locks all functions automatically after 3 mins. To disable, press and hold lockout button for 3 sec.



Alarm Silence
Mutes the audible alarm. (Visual light will not turn off until failure is resolved.)




Firm
Increases airflow for a firmer setting.



Soft
Decreases airflow for a softer setting.




Autofirm
Quickly inflates mattress to maximum firmness.



Fowler
Used when head section of bed is elevated. Increases airflow to the mattress.




Cycle Time
Increases or decreases the time of cycle between 3 to 90 minutes.



Mode
Press the Mode button to select Right Turn, Left Turn or Full Turn.



Low Pressure
Light will indicate when pressure is getting too low.



Pulsate
Press to begin Pulsation therapy



Power Failure
Light will indicate when power is no longer being provided to unit.

This chart is to be used as a reference ONLY. Final patient settings must be completed by the patient's caregiver.

Maintenance



CAUTION: The mattress requires regular maintenance to ensure performance and avoid premature wear, damage and injury.

Check the items on this chart at the indicated intervals. If any of the items are loose, worn, bent or distorted immediately have them checked and/or repaired by an authorized Sizewise technician. Frequent maintenance and servicing will improve performance and extend product life.

	Weekly	One Month	Three Months
Foam Filter	X		
HEPA Filter		X	
Top Cover		X	
Mattress Base		X	X
Mattress Connections			X
Control Unit Operation			X
Power Cord			


The following is an equipment safety checklist that can be used with the maintenance chart to maintain and service this product:

- Inspect top cover for punctures, rips, tears or damage.
- Inspect mattress base for punctures, rips, tears or damage.
- Connect the control unit and verify proper operation (if installed).
- Ensure air filter is clean and properly installed into control unit (if installed).
- Ensure mattress is clean/disinfected and patient ready.

All power cords are fastened in a manner to keep them free from moving or pinching parts. At any time parts are replaced, all cords should be secured into proper position to prevent damage.

Air Filter (Open cell foam filter)

The foam air filter on the back of the control unit must be cleaned weekly with disinfectant solution (see cleaning section). Replacement of the foam filter is recommended every 6 months.

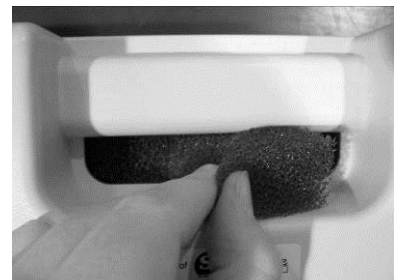

The filter is easily removed and reinserted through the gap in the back housing.

HEPA Filter

HEPA: (High Efficiency Particulate Air) filter.

NOTE: HEPA filters aid in contamination control for facilities. HEPA filters do not filter out gases and odor molecules such as chemical vapors and cigarette smoke.

NOTE: HEPA filter must be used in conjunction with the manufacturer supplied foam filter. DO NOT attempt to install HEPA filter without the original equipment foam filter.

NOTE: Ensure factory open cell foam filter is completely dry before placing HEPA filter in unit.

NOTE: The HEPA filter is to be installed in applicable models and pumps in conjunction with the next factory filter cleaning procedure.

Installation

NOTE: Installation and/or handling of HEPA filter requires PPE. Service personnel should wear a mask, gloves, and protective clothing to avoid exposure to possible contaminants.

NOTE: Tools are not required for installation of filter.

NOTE: Ensure unit is off and/or removed from power source prior to servicing or replacement of filter or HEPA filter.

- Locate and remove factory filter on the top and back of the case.
- Filter is easily removed and reinserted through the gap in the back of the case.
- Ensure HEPA filter is clean.
- Place HEPA filter on front of factory foam filter.
- Re-install filters in blower case.



HEPA Filter

Maintenance

NOTE: DO NOT MODIFY HEPA filter for installation. Order filter from Sizewise to receive filter with correct dimensions.

NOTE: DO NOT attempt to clean HEPA filters, as they are to be removed and replaced only.

- HEPA filters must be replaced monthly.
- Follow Installation procedure for monthly replacement of HEPA filter.

Troubleshooting

Problem	Cause	Solution
Reduced airflow	Possible clogged filter	Replace HEPA filter
Excessive noise	Possible obstruction Clogged filter	Ensure no obstructions Replace HEPA filter
Odor	Excessive contaminants in HEPA filter	Replace HEPA filter

Storage

If you store your product for more than 30 days, we recommend:

- Remove HEPA filter.
- Place HEPA filter in an air-tight plastic bag or plastic wrap ensuring filter is sealed to prevent exposure to outside contaminants.
- When you wish to operate product, reinstall HEPA filter.

Mattress Cleaning Instructions

WARNING and CAUTION:



It is recommended that gloves and protective clothing be worn at all times during cleaning and disinfecting.

DO NOT autoclave.

NOTE: Improper cleaning, rinsing or the incorrect use of cleaning agents can lead to premature fabric discoloration and breakdown of the fabric's fluid-resistance, stain-resistance and fabric strength. Properly rinsing all cleaning agents and disinfecting chemicals is a critical step in extending the life of covers on medical mattresses and support surfaces.

Over time, cleaning solutions may cause damage to the integrity of the fabrics used for support surfaces. Cleaning agents that are strong enough to be efficacious cleaners and disinfectants may cause degradation of the same fabrics on which they are being used.

To minimize the negative impact of cleaning agents:

- Contact time must be monitored and kept to the required time identified on the manufacturer's instructions.
- All cleaning solutions must be diluted in accordance with manufacturer's instructions.
- All covers must be rinsed after every cleaning cycle. Rinsing of the support surface (mattress) covers with clean water as the immediate step after the disinfection process is fundamental to extending the usable life of the covers.

NOTE: Only the outer cover of the mattress requires cleaning and maintenance. Disassembly of the support surface for maintenance of internal components is not recommended. DO NOT use harsh solvents or cleaners. Special care should be used to not puncture the mattress with needles or sharp instruments. This may result in loss of integrity of the mattress cover or internal components.

Recommended EPA Registered Disinfectants:

Wex-Cide 128 (Wexford Labs), EPA Reg. #34810-31

Equipment must be disinfected using an EPA registered, hospital-grade disinfectant, according to the manufacturer's recommendations for use.

Recommended Stain Remover(s):

Stain Away (ABC Compounding)

This stain remover is effective in removing most difficult stains and is intended to be used in its original concentration.

***Clostridium difficile* (C. diff) Prevention:**

Clorox Germicidal Wipes (Clorox Professional Products Company), EPA Reg. #67619-12

These pre-moistened wipes meet the CDC's recommendations for *Clostridium difficile* (C.diff) bacteria, after the manufacturer's recommended "wet contact time".

1. Perform hand hygiene using soap and warm water, or hand sanitizer, and then put on disposable gloves and eye protection.
2. Use wipes to wipe the top and front of head/footboards, hand controls and cords, side rails and mattress top cover, making sure to wipe between the mattress and side rails.
3. Change wipes often to ensure that surfaces remain wet with disinfectant for the manufacturer's required contact time. Used wipes are to be discarded in the trash.
4. Remove disposable gloves and discard in the trash; perform hand hygiene using soap and warm water, or hand sanitizer, and then remove eye protection.

To reduce the discoloration of fabrics and degradation of the sleep surface lining, surfaces must be thoroughly rinsed with clean, fresh water to remove chemical residues immediately after the manufacturer's recommended "wet contact time" has been reached. The use of bleach-based solutions must be avoided whenever possible.

Mattress Top Cover:

Personal Protective Equipment should always be used as directed by the disinfectant's Safety Data Sheet.

1. Prepare the disinfectant according to the manufacturer's recommendations.
2. Prepare a separate bucket of warm, fresh water to be used for rinsing the equipment after cleaning/disinfecting procedures are completed as instructed.
3. All surfaces of the mattress are to be wiped using a coarse cloth dampened with the disinfectant, prepared as directed by the manufacturer's recommendations, to remove organic material and visible soil.
4. Allow the mattress shell to remain wet with disinfectant solution for the manufacturer's recommended contact time.
5. Stains on the mattress top cover may be treated using an approved stain remover, according to the manufacturer's recommendations.
6. Rinse all surfaces of the mattress with fresh water and clean cloth to remove chemical and organic residue.

Laundry Instructions:

If additional cleaning is necessary, top covers may be removed and laundered using standard hospital disinfectant/detergent. **DO NOT use temperatures in excess of 120°F (49°C).**

1. Set washing machine to Regular Cycle.
2. Pre-soak with disinfectant/detergent in cold water for 10 minutes. **DO NOT USE HARSH SOLVENTS OR CLEANERS.**
3. Main wash cycle: 15 minutes (time dependent on soil level).
4. Rinse cycle: 5 minutes, minimum.
5. Spin/Drain cycle: 5 minutes, minimum.

After washing, the mattress top cover is to be air dried or dried in a dryer at very low or no heat to protect it from heat related damage.

Mattress Base:

1. Prepare the disinfectant according to the manufacturer's recommendations.
2. Prepare a separate bucket of warm, fresh water to be used for rinsing the equipment after cleaning/disinfecting procedures are completed as instructed.
3. All surfaces of the mattress are to be wiped using a coarse cloth dampened with the disinfectant, prepared as directed by the manufacturer's recommendations, to remove organic material and visible soil.
4. Allow the mattress shell to remain wet with disinfectant solution for the manufacturer's recommended contact time.
5. Stains on the mattress base may be treated using an approved stain remover, according to the manufacturer's recommendations.
6. Rinse all surfaces of the mattress with fresh water and a clean cloth to remove chemical and organic residue.
7. After washing, the mattress base must be allowed to air dry.

Air Therapy Internal Mattress Components:

1. Prepare the disinfectant according to the manufacturer's recommendations.
2. Prepare a separate bucket of warm, fresh water to be used for rinsing the equipment after cleaning/disinfecting procedures are completed as instructed.
3. Using a clean cloth dampened with the disinfectant solution, wipe all internal mattress surfaces, including the air cells, and allow to remain wet for the manufacturer's recommended contact time.
4. Rinse all surfaces of the air cells with fresh water and clean cloth to remove chemical and organic residue.
5. After cleaning, dry the internal air cells with a clean, dry cloth.
6. After all mattress components are dry, reinstall the top cover.
7. Store the mattress in a "clean" environment until the next use.

NOTE: Only the outer cover of the mattress requires cleaning and maintenance. Disassembly of the support surface for the maintenance of internal components is not recommended. DO NOT use harsh solvents or cleaners. Special care should be used to not puncture the mattress with needles or sharp instruments. This may result in loss of integrity of the mattress cover or internal components.

Cleaning Blood and Other Excretions:

Blood and other excretions should be wiped up while wet, if possible. These substances are more difficult to remove once they have dried to surfaces. Dried blood and other excretions are to be removed using ample disinfectant solution in order to moisten the substance and make it easier to clean.

Control Unit Cleaning Instructions:

NOTE: Hand clean only. DO NOT place in sterilization room or chamber.

1. Personal Protective Equipment should be used as directed by the Material Safety Data Sheet for the disinfectant.
2. Prepare the disinfectant according to the manufacturer's recommendations.
3. Turn off the control unit and disconnect it from all electrical power to avoid electrical shock.
4. When cleaning the control unit avoid excessive moisture, especially in areas where there are electrical connections and components, to prevent damage.
5. All surfaces of the control unit and the power cord are to be wiped using a coarse cloth, dampened with the disinfectant solution prepared as directed by the manufacturer's recommendations, to remove organic material and visible soil.
6. Allow the control unit to remain wet with disinfectant solution for the manufacturer's recommended contact time.
7. Rinse all surfaces of the control unit with fresh water and use a clean cloth to remove chemical and organic residue.
8. After cleaning, all surfaces are to be dried with a clean, dry cloth.

NOTE: DO NOT attempt to clean HEPA filters, as they are to be removed and replaced only.

Open cell foam filter ONLY

Control unit air filter (foam filter) must be cleaned weekly. Replacement of the control unit air filter is recommended every 6 months.

1. Remove the air filter located on the back of the control unit.
2. Clean with prepared disinfectant solution and allow to air dry.
3. Reinstall the filter when dry.

NOTE: To keep equipment working efficiently and effectively for an extended time period, it is essential to make sure the equipment is cleaned regularly and well maintained.

Safety Tips

Seven Zones of Bed Rail Entrapment

If the patient would have any clinical conditions that could result in risk of falling or improperly lying in bed, the bed should be left at its lowest setting and in flat position when not attended. The use of bed rails is recommended if they are available. There are seven zones of bed rail entrapment.



WARNING: Bed rail entrapment is a serious health risk that can result in serious injury or even death. Sizewise recommends the care provider be mindful of the FDA guidelines relevant to bed rail entrapment, as serious injury can result. These guidelines can be found on the FDA website. When using an Air Therapy system the care provider is responsible for ensuring the mattress properly fits the bed frame. It is also the care provider's ultimate decision whether or not to use bed rails with the patient.

Zone 1: Within the Rail

Zone 2: Under the Rail, Between the Rail Supports or Next to a Single Rail Support



Zone 3: Between the Rail and the Mattress

Zone 4: Under the Rail, at the Ends of the Rail


Zone 5: Between Split Bed Rails

Zone 6: Between the End of the Rail and the Side Edge of the Head or Footboard


Zone 7: Between the Head or Footboard and the Mattress End

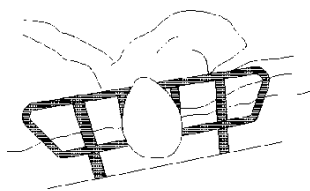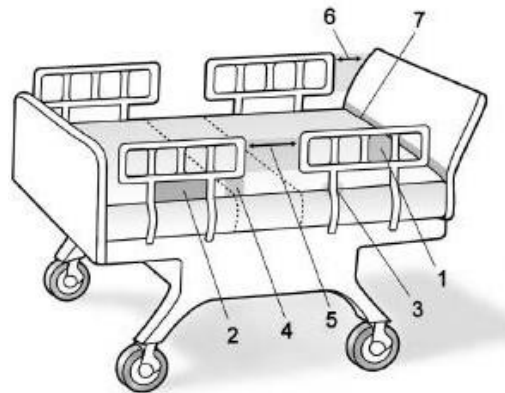


Zone One

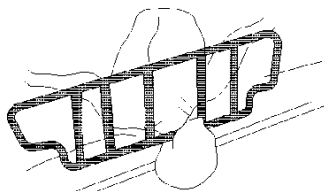


Zone Two



Zone Three

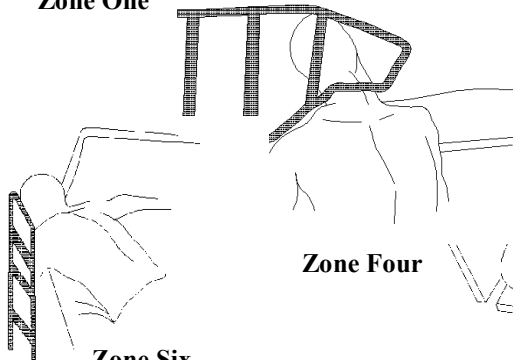

Zone Four

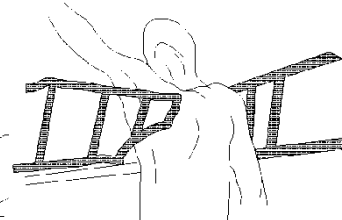

Zone Five



Zone Seven

Zone Six

Storage and Disposal

Keep the mattress in a clean dry area, away from heat or flames. Store the unit and mattress in a temperature range between 0°F (-18°C) and 95°F (35°C). Always store the surface flat on a clean, level surface. Avoid storage of other equipment on top of the support surface. DO NOT expose the control unit to humidity greater than 95%.

End-of life products must be disposed of properly according to local laws and regulations. Please contact Sizewise or your local authorities for disposal and recycling options.

Important Safety Instructions

Unpacking and Set-Up Instructions

- Keep out of direct sunlight.
- DO NOT expose to temperatures greater than 35°C (95°F) or below -18°C (0°F).
- DO NOT expose the Control Unit/Blower to humidity greater than 95%.
- (110V unit ONLY) Ensure the power cord is plugged into a properly grounded AC 110V outlet.

Safety Tips

- Medical equipment should not be used, stacked or located on or around equipment that may create electromagnetic interferences.
- Using other manufacturers' cables and accessories may affect EMC performance. Unauthorized use of these items will void warranty and could result in patient and/or user injury as well as damage to equipment or other property.
- The use of cables or accessories other than those for which the blower was designed or tested can significantly degrade emissions and immunity performance.
- DO NOT use the device if the power cord is cut, frayed or loosely connected.

Mattress Cleaning Instructions

- It is recommended that gloves and protective clothing be worn at all times during cleaning and disinfecting.
- DO NOT autoclave.
- The mattress requires regular maintenance to ensure performance and avoid premature wear, damage and injury.

Troubleshooting

- Only authorized personnel should engage in the troubleshooting process. Troubleshooting by unauthorized persons could result in personal injury or equipment damage.
- To avoid electrical shock, DO NOT open the Control Unit/Blower. Refer servicing to qualified personnel only.

Electromagnetic Compatibility (EMC)

The SIZEWISE STRATUS TURN® has been tested for compliance with the EMC requirements. The guidelines in this section will help to ensure the medical equipment will meet the requirements of the standard.



WARNING: Medical equipment should not be used, stacked, or located on or around equipment that may create electromagnetic inferences.

Emissions

This Control Unit/Blower has been type tested and has passed the requirements of CISPR 11. Observe the following recommendations to minimize radio frequency emissions in this section and the Electromagnetic Interference section.

Immunity

This Control Unit/Blower has been stringently tested for susceptibility to electromagnetic radiation over the frequency range 80 MHz to 2.5 GHz. The test was conducted on this Control Unit/Blower and passed the requirements of IEC 60601-1-2:2007.

All pins of connectors have passed ESD testing.

List of Cables & Accessories

Replacement parts, such as cables and accessories, must be purchased through Sizewise to ensure proper compliance requirements.



WARNING: Using other manufacturer's cables and accessories may affect EMC performance. Unauthorized use of these items will void warranty and could result in patient and/or user injury as well as damage to equipment or other property.

The use of cables or accessories other than those for which the Control Unit/Blower was designed or tested can significantly degrade emissions and immunity performance.

GUIDANCE AND MANUFACTURER'S DECLARATION

Company: Sizewise
Model: SIZEWISE STRATUS TURN®
Project Number: 3101425

**Table 201 Guidance and Manufacturer's Declaration - Emissions
All Equipment and Systems**

The blower is intended for use in the electromagnetic environment specified below. The customer or user of this blower should ensure that it is used in such an environment.

Emissions Test	Compliance	Electromagnetic Environment Guidance
RF Emissions CISPR 11	Group 2	The blower must emit electromagnetic energy in order to perform its intended function. Nearby electronic equipment may be affected.
RF Emissions CISPR 11	Class B	NOTE: The higher IMMUNITY TEST LEVELS specified for the HOME HEALTH CARE ENVIRONMENT are necessary due to the closer distances to certain electromagnetic sources than found in the professional healthcare facility environment. Examples include PORTABLE RF communications equipment such as mobile phones and amateur radio equipment.
Harmonics IEC 61000-3-2	Class B	
Flicker IEC 61000-3-3	Complies	

**Table 202 Guidance and Manufacturer's Declaration - Immunity
All Equipment and Systems**

The blower is intended for use in the electromagnetic environment specified below. The customer or user of the blower should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment Guidance
ESD IEC 61000-4-2	±6kV Contact ±8kV Air	A	Floors should be wood, concrete or ceramic tile. If floors are synthetic, the r/h should be at least 30%
EFT IEC 61000-4-4	±2kV Mains ±1kV I/Os	A	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1kV Differential ±2kV Common	A	Mains power quality should be that of a typical commercial or hospital environment.
Voltage Dips/Dropout IEC 61000-4-11	>95% Dip for 0.5 Cycle 60% Dip for 5 Cycles 30% Dip for 25 Cycles >95% Dip for 5 Seconds	A	Mains power quality should be that of a typical commercial or hospital environment. If the user of the blower requires continued operation during power mains interruptions, it is recommended that the blower be powered from an uninterruptible power supply or battery.
Power Frequency 50 Hz Magnetic Field IEC 61000-4-8	3A/m	A	Power frequency magnetic fields should be that of a typical commercial or hospital environment.

Table 204 Guidance and Manufacturer's Declaration - Immunity Equipment and Systems which are NOT Life-supporting

The blower is intended for use in the electromagnetic environment specified below. The customer or user of the blower should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment Guidance
<p>Conducted RF IEC 61000-4-6</p> <p>Radiated RF IEC 61000-4-3</p>	<p>3 VRMS .15 MHz to 80 MHz</p> <p>3 V/m 80 MHz to 2.5 GHz</p>	<p>$(V1)VRMS = 3$</p> <p>$(E1)V/m = 3$</p>	<p>Portable and mobile communications equipment should be separated from the blower by no less than the distances calculated/listed below:</p> <p>$D = (3.5/V1) (\text{SQRT } P)$</p> <p>$D = (3.5/E1) (\text{SQRT } P)$ 80 to 800 MHz</p> <p>$D = (7/E1) (\text{SQRT } P)$ 800 MHz to 2.5 GHz</p> <p>Where P is the max power in watts and D is the recommended separation distance in meters.</p> <p>Field strengths from fixed transmitters, as determined by an electromagnetic site survey, should be less than the compliance levels (V1 and E1).</p> <p>Interference may occur in the vicinity of equipment containing a transmitter.</p>

Table 206 Recommended Separation Distances between portable and mobile RF Communications equipment and the blower.

Equipment and Systems which are NOT Life-supporting

Recommended Separation Distances for the blower

The blower is intended for use in the electromagnetic environment in which radiated disturbances are controlled. The customer or user of the blower can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF Communications Equipment and the blower as recommended below, according to the maximum output power of the communications equipment.

$D = (3.5/\sqrt{P})$ (SQRT P)

$D = (3.5/E1)$ (SQRT P)

80 to 800 MHz

$D = (7/E1)$ (SQRT P)

800 MHz to 2.5 GHz

Compliance Level	Cond RF 3	Rad RF-800MHz 3	Rad RF - 2.5GHz 3
0.01	0.12	0.12	0.23
0.1	0.37	0.37	0.74
1	1.17	1.17	2.33
10	3.69	3.69	7.38
100	11.67	11.67	23.33

Troubleshooting



CAUTION: Only authorized personnel should engage in the troubleshooting process. Troubleshooting by unauthorized persons could result in personal injury or equipment damage.



WARNING: To avoid electrical shock, DO NOT open the control unit. Refer servicing to qualified personnel only.

If mattress is not inflating:

- Check that the hoses are not punctured, kinked or disconnected
- Check for proper connections from the hoses to the Control Unit/Blower. Make sure they are secure.
- Check air filters on back of the Control Unit/Blower and clean if necessary
- Ensure CPR function is in the closed position

If there is power loss:

- Check the ON/OFF switch
- Check power cord for any damage
- Unplug the Control Unit/Blower and check fuses located near the main ON/OFF switch. Replace fuse/s as necessary.
- Ensure unit is plugged into a Hospital grade receptacle.


NOTE: If the troubleshooting process does not solve the problem please contact a Sizewise representative for service.

Frequently Ordered Parts

The following is a list of parts that are frequently ordered for self-replacement and repairs. To aid in ordering parts, please use the provided product numbers given below for each part. The replacement of some parts not listed here may require sending in the unit to the manufacturer for repairs.



Connector – Connects from mattress to the control unit side panel. Allows air movement to inflate mattress.

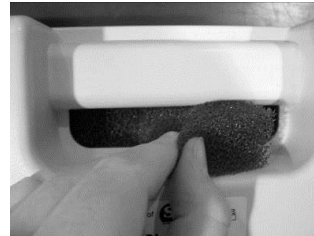

Filters – Removes dust and other particles from the air as it is pulled into the control unit.

Foam Filter Part Number
27400048
HEPA Filter Part Number
27400059



Power Cords – Grounded hospital grade power cord for providing power to the control unit. (**Note: Supplied only with 110V control units.**)



Hooks – Collapsible hooks that allow the unit to be hung on bed frame.



Product #
27502020

Brackets – Attach the hooks to the bottom case of the unit.

Product #
27502011

Sizewise Stratus Turn Mattress System

Product No. 61350016

Limited Product Warranty

PLEASE READ THESE WARRANTY TERMS AND CONDITIONS CAREFULLY BEFORE USING YOUR SIZEWISE PRODUCT. BY USING THE PRODUCT, YOU ARE CONSENTING TO BE BOUND BY THE FOLLOWING WARRANTY TERMS AND CONDITIONS.

LIMITED WARRANTY.

Sizewise warrants the above referenced product to be free from material defects in materials and workmanship for the warranty periods set forth below when the product is used and serviced properly in accordance with the specifications set forth in the Sizewise owner's manual in effect at the time of sale of the product, including without limitation compliance with the safe working load set forth therein. If there is no period of time specified below, the warranty period shall be ninety (90) days. The warranty periods commence on the invoice date of the original purchase. This warranty applies only against defects discovered within the warranty period and extends only to the original purchaser or designated original end user of the product ("Buyer"). Parts repaired or replaced under the terms of this warranty will be warranted for the remainder of the original warranty period only. Buyer is solely responsible for determining whether the products and services offered by Sizewise are appropriate for its intended use including use by Buyer's employees, invitees, contractors, representatives, third party beneficiaries, or any other person Buyer intends to use the product. Buyer acknowledges it has made the selection of the products based upon its own judgment and that the product is of a size, design, capacity, condition, quality, durability selected by Buyer. Buyer expressly disclaims any reliance upon any statements or representations made by Sizewise or any other party on its behalf except as otherwise specifically provided for in this Limited Product Warranty. Buyer acknowledges and agrees that the remedy in this warranty for the repair and replacement of defective product or part(s) shall constitute the sole remedy in the event of a defective product or part(s). **THE WARRANTY GIVES BUYER SPECIFIC LEGAL RIGHTS, AND BUYER MAY ALSO HAVE OTHER RIGHTS THAT VARY FROM STATE TO STATE.** Sizewise's obligations under this warranty are limited as set forth below.

WARRANTY PERIOD AND COVERAGE.

SW™ STRATUS TURN MATTRESS SYSTEM

- 2 yr. on control/pump unit
- 1 yr. limited on mattress
- 90 days on top cover
- 1 yr. on electronics

CONDITIONS AND RESTRICTIONS.

This warranty is valid only in accordance with the conditions set forth below:

- The warranty applies to this Sizewise product only while:
 - it remains in the possession of the Buyer and proof of purchase is demonstrated,
 - it has not been subjected to accident, misuse, abuse, improper service, or modification,
 - claims are made within the warranty period.
- This warranty does not apply to any other products or devices sold separately regardless of whether used with this product. Such other products or devices will be subject to the separate limited product warranty set forth in the user manual for such product or device.
- Sizewise's sole liability shall be discharged by replacing or repairing, at Sizewise's option, the product or its part or parts which are determined by Sizewise to be defective under normal and proper use during the warranty period.
- Buyer shall notify Sizewise or the authorized Sizewise dealer immediately but in no event more than seven (7) days after the date of discovery of any alleged defect by contacting Sizewise Parts and Services at 1-800-814-9389 Monday through Friday 8am – 5pm CST.
- If the product or part should be returned to Sizewise, a return authorization number (RA#) must be obtained by Buyer from Sizewise. The RA# will be valid for 21 days from the date it is issued.
- Buyer is responsible for any shipping, freight, handling, pickup or delivery charges or fees including without limitation any expediting fees involved with the delivery of the defective product or parts to Sizewise's factory for repair or replacement.
- If on-site technical service is required, a service representative will be dispatched during Sizewise's standard service hours Monday through Friday 8am-5pm CST and provided the product is located within Sizewise's serviceterritory.
- If Sizewise determines the problem with the product or part(s) is a result of defective material or workmanship, the

Sizewise Stratus Turn Mattress System

Product No. 61350016

Limited Product Warranty

product or part will be replaced or repaired at the discretion of Sizewise, and at no charge to the Buyer however subject to the limitations and exclusions of this Limited Product Warranty.

- At the election of Sizewise, replacement parts may be new or refurbished; and Sizewise reserves the right to substitute materials if original materials are no longer available.
- If Sizewise determines the product or part that Buyer has requested warranty services on are not covered by the warranty for any reason including without limitation because it is outside of the warranty period, excluded from the warranty or the warranty is void, Buyer shall pay for the repair or replacement services, including parts and labor performed by Sizewise at Sizewise's prevailing time and material rates plus freight and delivery.
- If Buyer declines the repair or replacement service upon notice from Sizewise it is not covered under warranty, Buyer shall reimburse Sizewise for all costs from investigating and responding to Buyer's request.
- Any costs to Buyer as referred to herein shall be at Sizewise's prevailing time and material rates plus any freight and delivery charges incurred by Sizewise.
- Any assistance provided by Sizewise outside the terms of this warranty does not waive the limits of this warranty.
- Sizewise does not pay labor outside the United States.
- Any description of Sizewise's products is for identification purposes only and is not an express warranty.
- Loaned products, demo or sample products and/or consumable products including without limitation batteries and sheets are furnished to Buyer on an "AS IS WITH ALL FAULTS" basis.

EXCLUSIONS AND LIMITATIONS.

This Limited Product Warranty shall not apply to, and Sizewise shall have no obligation to make repairs, replace or correct products including any part or parts of the product as the result of Sizewise's determination of any of the following:

1. Software (PROM) or firmware version upgrades or updates or any other changes and/or any outages, interruptions, delays, attacks, malware, or any other technology or viruses on such software or firmware or Buyer's network, if applicable to this product.
2. Normal wear and tear of the product including without limitation normal discoloring, body impressions on mattresses or loss in some resiliency, if applicable to this product, and cosmetic items, consumable items including without limitation mattresses, casters, sheets, handsets and batteries.
3. Damage due to improper transport, storage, installation, maintenance, use, repair or failure to follow Sizewise's instructions or procedures as detailed in the owner's manual.
4. Damage or malfunctions resulting from work performed by service providers not authorized by Sizewise.
5. Repairs performed on a Sizewise product or parts missing a serial number or with a serial tag that has been altered, tampered with or defaced in any manner.
6. Service calls to correct installation of the product unless installed under contract by Sizewise or its partners and in which event the terms of the service contract only shall apply to service installation corrections.
7. Shipping, freight, handling, pickup and delivery charges or fees involved with delivery of the products and or part(s) to Sizewise's factory for repair or replacement and returning the replacement or repaired products and/or parts to Buyer.
8. Any labor costs incurred beyond the applicable labor warranty period.
9. Damage or product failure from causes external to the product or part(s) including without limitation power or electric failure or surges, electrical wiring not in compliance with electrical codes or Sizewise owner's manual specifications.
10. Damage caused by failure to provide reasonable and necessary maintenance as outlined in the owner's manual.
11. Damage caused by the use, misuse, negligence, loss, abuse of the product or any parts by Buyer including without limitation any third party beneficiaries, end user or others persons Buyer intends to use the product, including without limitation (except Sizewise or an authorized Sizewise service provider):
 - a. exceeding the safe working load on this product or any specific weight capacity for a part,
 - b. cleaning upholstery or fabrics with harsh chemicals, or bleach, outside the recommended cleaning guidelines,
 - c. altering, tampering with, or modifying in any manner without the express written consent of Sizewise any part(s) or structural components or appurtenances of the products,
 - d. use of the product or part(s) in a manner for which it is not designed or in any manner inconsistent with the information set forth in the Sizewise owner's manual including without limitation use with other devices or ancillary products for which it was not intended.
12. Exposure of the product or part(s) to, whether foreseen or unforeseen, accident, acts of God, or natural causes (such as natural disasters, fire, flood, wind, water or powerfailures, acts or threats of terrorism).

Sizewise Stratus Turn Mattress System

Product No. 61350016

Limited Product Warranty

13. Operation of the product beyond its normal useful life.
14. Buyer's failure to show proof of purchase.
15. Products or items not manufactured by Sizewise. Rather for products or items obtained by Sizewise from an original manufacturer or third party supplier Sizewise may assign to the Buyer any warranty rights in such products or items that Sizewise may have from the original manufacturer or third party supplier, to the extent such assignment is allowed by the original manufacturer or third party supplier.

DISCLAIMER AND RELEASE.

The warranties provided herein are the exclusive warranties given by Sizewise and supersede any prior, contrary or additional representations or warranties, whether oral or written. **EXCEPT FOR THE EXPRESS WARRANTIES IN THIS LIMITED PRODUCT WARRANTY, SIZEWISE DISCLAIMS ANY AND ALL OTHER WARRANTIES WHETHER EXPRESS OR IMPLIED WARRANTIES, INCLUDING, WITHOUT LIMITATION, ANY WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE OR NON-INFRINGEMENT, AND ANY WARRANTIES ARISING FROM COURSE OF DEALING, USAGE OF TRADE, OPERATION OF LAW OR OTHERWISE WITH RESPECT TO ANY PRODUCT, SERVICES, PARTS INCLUDING REPAIRED OR REPLACED PRODUCTS AND PARTS. ARE HEREBY DISCLAIMED AND EXCLUDED. Sizewise ALSO HEREBY DISCLAIMS AND EXCLUDES ALL OTHER OBLIGATIONS OR LIABILITIES, EXPRESS OR IMPLIED, ARISING BY LAW OR OTHERWISE, WITH RESPECT TO ANY NONCONFORMANCE OR DEFECT IN ANY PRODUCT OR PART(S), INCLUDING BUT NOT LIMITED TO: (A) ANY OBLIGATION, LIABILITY, RIGHT, CLAIM OR REMEDY IN TORT, WHETHER OR NOT ARISING FROM THE NEGLIGENCE OF SIZEWISE OR ITS SUPPLIERS (WHETHER ACTIVE, PASSIVE OR IMPUTED); AND (B) ANY OBLIGATION, LIABILITY, RIGHT, CLAIM OR REMEDY FOR LOSS OF OR DAMAGE TO ANY PRODUCT OR PART(S). THIS DISCLAIMER AND RELEASE SHALL APPLY EVEN IF THE EXPRESS WARRANTY SET FORTH ABOVE FAILS OF ITS ESSENTIAL PURPOSE.**

Exclusive Remedies.

For any product described above that Sizewise determines to have failed to conform to its warranty, Sizewise will provide, at its option, one of the following:

- (1) repair;
- (2) replacement; or
- (3) refund of the purchase price.

Sizewise Limited Product Warranty service may be obtained by contacting Sizewise or the authorized dealer from whom Buyer purchased the item. Sizewise compensates only Sizewise authorized service providers for warranty trips within their normal service area to repair commercial products at the customer's location.

THESE SHALL BE THE SOLE AND EXCLUSIVE REMEDIES OF THE BUYER FOR ANY BREACH OF WARRANTY.

EXCLUSION OF CONSEQUENTIAL AND INCIDENTAL DAMAGES.

SIZEWISE AND/OR ITS SUPPLIERS SHALL HAVE NO OBLIGATION OR LIABILITY, WHETHER ARISING IN CONTRACT (INCLUDING WARRANTY), TORT OR ANY OTHER LEGAL THEORY (INCLUDING ACTIVE, PASSIVE, OR IMPUTED NEGLIGENCE AND STRICT LIABILITY), OR OTHERWISE, FOR DAMAGE TO THE PRODUCT INCLUDING PART(S), PROPERTY DAMAGE, DEATH, PERSONAL INJURY, LOSS OF USE, GOODWILL, REVENUE OR PROFIT, COST OF CAPITAL, COST OF SUBSTITUTE PRODUCT, ADDITIONAL COSTS INCURRED BY BUYER (BY WAY OF CORRECTION OR OTHERWISE) OR ANY OTHER INCIDENTAL, SPECIAL, INDIRECT, COMPENSATORY OR CONSEQUENTIAL DAMAGES, INCLUDING WITHOUT LIMITATION WHETHER RESULTING FROM NONDELIVERY, USE, MISUSE OR INABILITY TO USE THE PRODUCT, SERVICES OR PART(S). THIS EXCLUSION APPLIES EVEN IF THE ABOVE WARRANTY FAILS OF ITS ESSENTIAL PURPOSES AND REGARDLESS OF WHETHER SUCH DAMAGES ARE SOUGHT FOR BREACH OF WARRANTY, BREACH OF CONTRACT, NEGLIGENCE, OR STRICT LIABILITY IN TORT OR UNDER ANY OTHER LEGAL THEORY. SIZEWISE LIABILITY SHALL BE LIMITED TO THE AMOUNT PAID BY BUYER FOR THE RELEVANT PRODUCT. SOME STATES DO NOT ALLOW THE EXCLUSION OR LIMITATION OF INCIDENTAL OR CONSEQUENTIAL DAMAGES, SO THE ABOVE LIMITATION AND EXCLUSION ON SUCH MAY NOT APPLY.

EXTENDED WARRANTY. If the product covered under the Limited Product Warranty set forth herein had from Sizewise an extended warranty option made available only at the time of the Buyer's original purchase from Sizewise, Buyers who then also purchased such extended warranty, and have proof of such purchase, may extend the warranty period stated above in the Limited Product Warranty on parts, electronics, frame and labor relating to parts, electronics and frame repairs, as applicable,

Sizewise Stratus Turn Mattress System
Product No. 61350016
Limited Product Warranty

for an additional one (1) or two (2) years, whichever extension is purchased by Buyer (“extended warranty period”). Other than the extension on the warranty period, all other terms of the limited product warranty including without limitation the conditions and restrictions, exclusions and limitations, disclaimer and release, and exclusion of consequential and incidental damages of the original limited product warranty apply during the extended warranty period. For the purpose of clarity an extended warranty is not available where the original warranty period is less than one (1) year, and an extended warranty may only be purchased by Buyer at the time of the original purchase of the product from Sizewise.

To make a warranty claim, contact:

SIZEWISE
8601 MONROVIA
LENEXA, KS 66215
1-800-814-9389 Monday through Friday 8am-5pm CST

Complete this portion and keep for your records.

Purchased From: Sizewise

Product/model: _____

Serial number: _____



8601 Monrovia Street
Lenexa, KS 66215

800-814-9389
sizewise.com

*Sizewise is a registered trademark of Sizewise Rentals, LLC.
All specifications, equipment, and prices are subject to change without
notice. Photos and drawings are representative of the products and may
vary slightly from actual production models.*